



# Advances in drop and bubble profile analysis tensiometry

Aliyar Javadi<sup>1</sup>, Libero Liggieri<sup>2</sup>, Eugene V. Aksenenko<sup>3</sup>,  
Georgi G. Gochev<sup>4,5</sup> and Reinhard Miller<sup>6</sup>

## Abstract

Profile analysis tensiometry (PAT) with drops and bubbles is a successful methodology to characterize liquid–fluid interfaces. Questions about the most suitable size of drops and bubbles have been solved now on the basis of dimensionless numbers. The consideration of the standard deviation between measured and calculated liquid profiles as a sensitive measure for the applicability of PAT provides a tool for its correct use. For solutions of highly surface-active compounds, bulk depletion effects can cause systematic errors in the analysis of adsorption kinetics, equations of state, and the visco-elastic interfacial behavior of liquid adsorption layers. Great progress has been made in measurements of interfacial dilational rheology with large amplitude perturbations providing additional information about structure and dynamics of complex adsorption layers. Also, first attempts are successfully made to use artificial intelligence (AI) to enhance the efficiency of PAT applications. Thus, PAT has established a solid position in surface science.

## Addresses

<sup>1</sup> Institute of Fluid Dynamics, Helmholtz-Zentrum Dresden-Rossendorf (HZDR), Bautzner Landstraße 400, D-01328 Dresden, Germany

<sup>2</sup> CNR-Institute of Condensed Matter Chemistry and Technologies for Energy, Unit of Genoa, 16149 Genoa, Italy

<sup>3</sup> Institute of Colloid Chemistry and Chemistry of Water, National Academy of Sciences of Ukraine, 03680 Kyiv (Kiev), Ukraine

<sup>4</sup> Jerzy Haber Institute of Catalysis and Surface Chemistry, Polish Academy of Sciences, Krakow, Poland

<sup>5</sup> Institute of Physical Chemistry, Bulgarian Academy of Sciences, 1113 Sofia, Bulgaria

<sup>6</sup> Institute of Condensed Matter Physics, Technical University Darmstadt, D-64289 Darmstadt, Germany

Corresponding authors: Miller, R ([reinhard.miller@pkm.tu-darmstadt.de](mailto:reinhard.miller@pkm.tu-darmstadt.de)); Javadi, A ([javadi.aliyar@hzdr.de](mailto:javadi.aliyar@hzdr.de))

Current Opinion in Colloid & Interface Science 2024, 73:101846

This review comes from a themed issue on **Surface Analysis Techniques (2024)**

Edited by **Libero Liggieri** and **Reinhard Miller**

For a complete overview see the [Issue](#) and the [Editorial](#)

<https://doi.org/10.1016/j.cocis.2024.101846>

1359-0294/© 2024 The Authors. Published by Elsevier Ltd. This is an open access article under the CC BY-NC license (<http://creativecommons.org/licenses/by-nc/4.0/>).

## Keywords

Surface tension, Interfacial tension, Dilational interfacial visco-elasticity, Drop profile analysis tensiometry, Gauss-Laplace equation, Surface layer characterization.

## Introduction

Drop and bubble profile analysis tensiometry (PAT) is an old and at the same time novel methodology. Historically, the determination of the profile of a sessile and pendent drop or buoyant bubble was a rather time-consuming method due to the need of printing the photo taken from the drop or bubble and its analysis based on more or less accurate determination of geometric measures and subsequent complicated manual calculations with a pencil and a sheet of paper [1,2]. Hence, the surface tension  $\gamma$  of a liquid was available, but it had a rather low accuracy. Meanwhile, due to the availability of electronic cameras and powerful computers, this method evolved into the most frequently applied technique for systematic studies of liquid interfaces. The key progress was achieved by Neumann and his team in the eighties of the last century [3], who for the first time set up an instrument based on an electronic camera connected at that early time to a workstation [4]. The concept of this Axisymmetric Drop Shape Analysis (ADSA) represented the state of the art over many years until “normal” personal computers provided sufficient capacity to manage all required work like image acquisition, profile detection and fitting the Gauss-Laplace equation (GLE) to this profile, so that many different commercial instruments as well as single laboratory set-ups appeared. The first drop profile instrument based on a normal personal computer was the one by Benjamins et al. [5], allowing already to perform drop oscillations for measuring the dilational visco-elasticity of surface layers. Nowadays, even simple smartphones are able to manage the required job and provide data about the surface tension of liquid interfaces [6]. One of the great advantages of oscillating drops or bubbles is that one can generate almost ideal

Given the role as Guest Editor, Reinhard Miller, Libero Liggieri had no involvement in the peer review of the article and has no access to information regarding its peer-review. Full responsibility for the editorial process of this article was delegated to Marie Pierre Krafft.

expansions and compressions, avoiding any additional shear deformation. Such experiments are difficult to perform with other types of instruments and require special designs and protocols as proposed in Ref. [7].

A number of new findings were published during the last few years, dealing with the applicability, accuracy, and functionality of profile analysis tensiometry. One of the most frequently asked questions refers to the optimum size of drops or bubbles required for experiments with high accuracy [8,9]. Moreover, we know that the profile analysis has a limited range of applicability when used under highly dynamic conditions or when the drops/bubbles are covered, for example, by a crosslinked polymer membrane rather than an adsorbed layer. In both cases, an equilibrium balance of surface and bulk forces is required to measure physical quantities, and remarkable errors can be obtained when this balance is not in equilibrium. Mahmoudvand et al. [10] demonstrated that the standard deviation between experimental and theoretical drop/bubble profiles calculated via the GLE is a very powerful criterion to decide about the applicability of PAT. Some particular experiments have also been performed with the same surfactant solutions using the profile of a drop or bubble, respectively. Actually, no systematic differences should be expected, however, for solutions of very low surfactant bulk concentrations  $c$ , remarkably higher  $\gamma$  values are measured with solution drops as compared to bubbles, and the equilibrium values are established after significantly longer adsorption times, which can be explained by bulk depletion due to adsorption at the surface [11].

In addition to improvements in the methodology of PAT, quite a number of new experimental protocols have been proposed during the last few years. This includes not only experiments based on large amplitude oscillations [12] but also classical PAT experiments with constant drop/bubble size or with small amplitude oscillations, such as those proposed by Dowlati et al. [13] or Ashoorian et al. [14]. These new approaches at a broader range of experimental conditions as well as how AI can help increase the efficiency and reduce the required experimental efforts for obtaining reliable experimental data nowadays even via deep learning methods [15,16], will be discussed here. Note, there are also other interfacial methods, such as the spinning drop tensiometry, which was further developed so that reliable interfacial layer oscillations can be performed even at very low values of the interfacial tension [17].

### Improvements of the experimental performance

The question is: what is the optimum drop/bubble size for PAT to get the most accurate results was discussed in Refs. [8,9]. Berry et al. proposed to use the Bond number  $Bo$  or Worthington number  $Wo$  to estimate the

optimum drop size for accurate measurements. Both numbers contain the surface/interfacial tension so that the optimum drop size depends on this unknown parameter:

$$Bo = \frac{\Delta\rho g R_0^2}{\gamma} \quad (1)$$

$$Wo = \frac{\Delta\rho g V}{\gamma \pi D} \quad (2)$$

with  $R_0$  and  $V$  being the radius of curvature and volume of the drop, respectively, and  $D$  the diameter of the needle at which the drop is formed. The larger the values of  $Bo$  and  $Wo$ , the more accurate are the data obtained from PAT. However, the optimum values of  $Bo$  or  $Wo$  can hardly be determined prior to experiments. There are also situations in which the Bond number fails to determine the optimum drop size so that Yang et al. proposed a new dimensionless number instead, the Neumann number  $Ne$  [9]

$$Ne = \frac{\Delta\rho g R_0 H}{\gamma} \quad (3)$$

where  $H$  is the height of the drop. A perfect way to estimate the most suitable drop size for reaching the highest accuracy, however, does not exist anyway when surface-active compounds are present in the system as then  $\gamma$  is a function of time and decreases during the experiment, i.e. the corresponding values of all dimensionless numbers increase so that the drop with an initially optimum size would detach.

With respect to measurements of dynamic interfacial phenomena, the speed of the technique is essential. Thus, it is a new milestone to have this novel way of solving the Laplace equation via a deep learning procedure that enhances the speed of measurements and allows to correct insufficient experimental conditions [15].

It is worth mentioning that recently even the use of a smartphone [6] was proposed and demonstrated that surface tension measurements are doable even with simple and easily accessible parts. Although this achievement is impressive, the accuracy and functionality of such self-made instruments are far below the possibilities reached by commercial products of most of the leading companies. In particular, the various preprogrammed experimental protocols available with these instruments are of enormous value, the simplest of which is, for instance, the option to keep the size of a drop or bubble constant over a certain time interval.

As one can see from the definition of the dimensionless numbers by Eqs. (1)–(3), any inaccuracies in the parameter values for  $g$  and  $\Delta\rho$  lead to direct errors in the measured values for  $\gamma$ . Thus, the value for  $g$  should be

the one valid for the place of measurements. Most critical is the value for  $\Delta\rho$ . For interfaces between two liquids with almost the same density, as it is the case for water/silicon oil system, small errors in the used density values could lead to enormous errors in the final determined interfacial tension.

The application of PAT to a number of systems for obtaining reliable experimental results is sometimes rather questionable. The use of the standard deviation (STD) of fitting an experimental profile by the GLE as a criterion for acceptable conditions can be an essential help. The authors in Ref. [10] show that during fast drop size changes, the STD value can increase significantly, well above the accuracy of profile fitting by the GLE, which is typically in the range between 0.1 and 1.0  $\mu\text{m}$  for modern charge-coupled device (CCD) cameras. STD also increases strongly, by one or even two orders of magnitude, when the surface of a drop is covered not by a simple surfactant adsorption layer but by a compressed nanoparticle layer subject to collapse. Figure 1 shows the dynamic interfacial tension  $\gamma(t)$  (IFT) for the interface between hexane and an aqueous 0.09 mM Cetyltrimethylammonium Bromide (CTAB) solution containing 1 wt% of silica nanoparticles (with a diameter of 9 nm). The experimental protocol consists of a first constant drop volume of  $V = 20 \text{ mm}^3$  followed by a large decrease and a subsequent increase back to the original drop size. Due to the compression,  $\gamma(t)$  decreases strongly down to about 5 mN/m.

When  $\gamma(t)$  reaches values below 10 mN/m, an irregularity is observed, caused by the surface layer collapse. At the same moment, the standard deviation STD starts to increase from values around 1  $\mu\text{m}$  up to 30  $\mu\text{m}$ , pointing at the fact that the drop has no longer a Laplacian shape. When increasing the drop size again

back to its original value, the IFT increases again and returns back to values close to those measured before starting the compression, and also the STD decreases back to typical values of about 1  $\mu\text{m}$ . We can conclude that only when the STD is sufficiently small, the PAT method is applicable and provides meaningful IFT data, while for STD values larger than about 5  $\mu\text{m}$ , the resulting IFT data are only apparent values.


Similar effects were observed for aqueous dispersions of glass beads with diameters between 2  $\mu\text{m}$  and 35  $\mu\text{m}$ . Due to the sedimentation of the glass particles within the drop, its shape becomes deformed, and hence erroneous surface tensions are obtained from PAT [18]. The values of the measured surface tensions depend on the size and amount of added glass beads and are therefore only apparent values.

As generally accepted, the use of PAT is possible when interfaces are in a mechanical equilibrium and the adjacent bulk phases are essentially homogeneous. Otherwise, as shown above [10], the obtained results can be erroneous. In Ref. [19], PAT was applied to emulsion systems containing biosurfactants. It was observed that the surface tension decrease caused by the presence of biosurfactants disappeared step by step with increasing solution age, while parallel measurements with a Wilhelmy plate tensiometer (WPT) showed a stable, strong surface tension decrease of the biosurfactants. It turned out that the results of both methods were erroneous due to the presence of an oil component emulsified by the biosurfactants, leading in the case of PAT experiments to a “deactivation” and in the case of the WPT experiments to an overestimation of the biosurfactants’ surface activity. A correct, careful handling of the studied liquid would have, however, allowed to reach correct results with both methods.

PAT is usually practiced with pendent drops or buoyant bubbles, as from experienced users we know that these modes are more accurate and easier to handle than experiments with sessile drops. Anyhow, a new data handling package has been developed by Tang and Cheng [20] that allows for reliable measurements of surface and interfacial tensions with sessile drops or bubbles. However, the handling of a number of experimental routines, such as drop oscillations, appears difficult to be realized, so some traditional geometries with pendent drops/buoyant bubbles remain superior.

As for many other technology fields, machine learning (ML) and AI approaches are opening interesting perspectives in the improvement of tensiometry techniques. For PAT, such an approach relies on the training of an artificial neuronal network using a large set of numerically-generated drop shapes via the GLE, and based on non-dimensional quantities like the above-defined dimensionless numbers  $B_0$ ,  $W_0$ , or  $Ne$  in order to obtain shapes

Figure 1

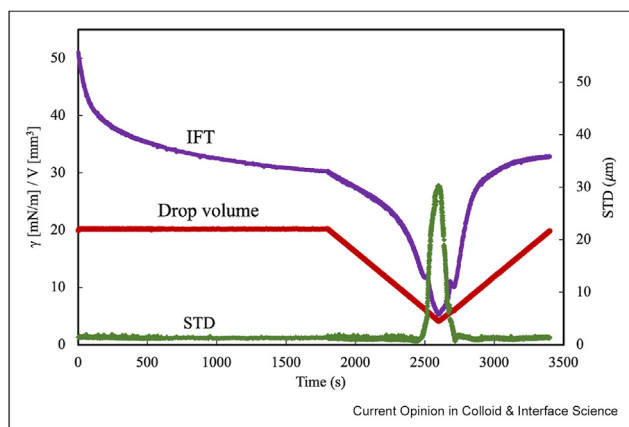

Change of interfacial tension  $\gamma(t)$  and drop volume  $V(t)$  with time and the corresponding STD values for an aqueous nanofluid/hexane interface (details are given in the text); redrawn from Ref. [10].

independent from the specific experimental magnifications and constraints. This approach was adopted by Kratz [15], who, in addition, discusses the performance of the method based on the use of the  $W_0$  number and the possibility of applications to the analysis of time-dependent series of images, such as those needed to measure the dilational surface rheology. The paper provides in addition an interesting introduction to the principles of capillarity for pendant drops, based on stability and bifurcation concepts. Soori et al. [21] have tested the performance of their ML approach for the analysis of pendant drop images to predict the surface tension of water-alcohol mixtures of unknown composition. A further important contribution in this area was made by Hyer et al. [16], who report the outstanding performance of their implemented convolutional neural network, able to analyze pendant drop images within 1.5 ms, obtaining surface tension values with absolute errors of the order of 0.15 mN/m. They have also tested the robustness of their algorithm, showing the possibility to keep the error below 0.3 mN/m in the inferred surface tensions from images of challengingly poor quality, caused, for example, by blurring, poor focus or vertical misalignment. With different degrees of performance, superior computational speed and robustness, as compared with the classical GLE best-fit analysis, are common crucial characteristics of ML approaches developed so far. In addition, these algorithms provide the possibility to infer the surface tension also in conditions where the mechanical equilibrium for axisymmetric drops is not fully respected. Thus, drop shape analysis based on ML carries an important potential in respect to studies of dynamic interfacial phenomena or for applications in industrial plants that could benefit from real-time measurements at a large number of points distributed along the production lines. Given the speed of developments in the area of ML, the described performances will likely improve even more in a short time, and the implementation of these algorithms in commercial instruments are likely going to occur soon. Besides the specific performances, the use of AI and ML thus represents a new milestone for drop profile analysis tensiometry, possibly comparable to the revolution associated with the introduction of computer-assisted profile analysis about 50 years ago [3].

### New experimental protocols for profile analysis tensiometry

The methodology of PAT, including drops as well as bubbles, is suitable for a broad variety of experiments. Zuo with his team showed, for example, that via drop oscillations various types of waveforms can be generated [22,23] and used for interfacial studies. Due to its flexibility, PAT allows also the characterization of rather complicated surface-active systems, such as asphaltenes and their efficiency in stabilizing emulsions [14], for dispersions with solidifying surface layers [24], for the

characterization of ionic liquids [25], or for the quantification of interactions between surfactants and particles or proteins in liquid interfacial layers [13,26].

For practical applications in oil fields, measuring instruments have to fulfill particular conditions. A Python-based image processing technique was used in Ref. [27] to set up an automated analysis protocol to determine surface and interfacial tensions as well as contact angles, which is much faster than the classical fitting procedures of drop profiles via the GLE, however, with a much lower average accuracy. The use of artificial intelligence, as described in Ref. [16] for a time-saving use of PAT, and as demonstrated in other recent papers [28–30], will become more widespread and make existing methods and experimental protocols easier and more efficient, however, the accuracy described so far is still much lower than that reached by a conventional analysis.

Surface tension measurements at high atmospheric pressures and elevated ambient temperatures are still a great challenge. Most suitable for such measurements seems to be the PAT method. Barrabino et al. demonstrated that, for example, studies at the interface between liquid CO<sub>2</sub> and water are possible with PAT when a particular measuring cell is available [31]. Measurements, which are of importance for tertiary oil recovery based on the injection of CO<sub>2</sub> into the rocks, are feasible up to 1300 bar and 200 °C, and in addition to standard dynamic interfacial tension measurements, drop oscillation experiments for obtaining the dilational viscoelasticity of the respective liquid interfaces were possible [32]. This methodology is also essential for fundamental studies on the capture and storage of carbon in the underground [33].

PAT in a sessile drop mode has been used during the last 30 years to measure the surface tension of molten metals and alloys to design high-performance materials. The major drawback in these set-ups was the reactivity of the melt with the crucibles at the high temperatures. Thus, more recently, set-ups based on the utilization of pendant drops have appeared [34], which warrants measurements in nearly container-less conditions and allows therefore investigations of the interfacial properties of liquid metals even at very high temperatures [35].

The group of Lin performed a number of very interesting experiments with a bubble profile analysis tensiometer using randomly appearing fluctuations in the closed system of the buoyant bubble caused by the temperature control loop [36]. The temperature fluctuations caused a volume change of the bubble and hence a change in the surface area  $A$ , leading consequently to surface tension changes. An accurate analysis

of the observed minute area perturbations and the corresponding surface tension changes as a result allowed to determine the dilational visco-elasticity in the respective moment of the experiment, leading finally to a time dependence of the visco-elasticity. In Ref. [37], the authors used this protocol, actually consisting of a buoyant bubble under temperature control, to determine the establishment of the equilibrium adsorption layer of proteins, using the observed changes in the dilational surface visco-elasticity. This type of experiments allowed to accurately determine the time required by a protein adsorption layer to reach the equilibrium state. The equilibrium state characterized by constant dilational surface viscosity data is reached much later than it is typically concluded from the constant dynamic interfacial tensions [38].

The analysis of surface tension changes caused by temperature fluctuations, used to determine the dilational visco-elasticity of fluid interfaces is a new approach and represents a complementation of experiments with formed harmonic oscillations of pendent drops/buoyant bubbles. It is worth mentioning here that this type of experiment has limits in the applied frequency, i.e. too high frequencies lead to wrong experimental results. In Ref. [39], it was for example shown that oscillations at a frequency of 1 Hz, which is almost one order of magnitude higher than the allowed maximum frequency, the surface layer of a pure water drop becomes visco-elastic, which is physically nonsense. A similar problem arises when the profiles of drops or bubbles are captured under dynamic conditions, for example, immediately after drop/bubble formation or during a growth process. Also under these conditions, the resulting values of surface or interfacial tension are erroneous, as shown in Ref. [40].

Although the majority of measurements of the dilational surface and interfacial rheology are performed presently by PAT with oscillating drops and bubbles, Zamora *et al.* [17] and Marquez *et al.* [41] proposed to use also the spinning drop method. This is of particular importance for studies of oil/water microemulsions where the measured tensions are extremely low and the classical PAT technique fails. The application of the oscillating spinning drop methods is particularly important for the tertiary oil recovery, although the analysis of the relaxation mechanisms in a spinning tube is very difficult due to the complex structure of the liquid flow which is in dynamic rotation and not in a quiescent equilibrium state as it is the case in PAT measurements.

The experimental investigations of the mechanical behavior of fluid interfaces are often complicated by the need to accurately separate the impact of the interface from that of the adjacent bulk phases. Moreover, while interfacial shear rheology can be studied via more or less ideal shear deformation experiments, in dilational

interfacial rheology it is much more difficult to produce ideal expansions and compressions without a remarkable shear contribution. Moreover, in many cases, the interfacial layers are not perfectly homogeneous and sometimes even show particular structures, so that specific assumptions are to be made for a correct analysis of experimental data. In Ref. [42], an overview of the computational interfacial rheology is given that allows to analyze systems, in particular of liquid–fluid interfaces, covered by polymers, particles or any other molecular or supramolecular surface-active materials. The presence of complex structured interfacial layers complicates the correct data analysis via the GLE due to the presence of additional stresses of different nature, considered in detail by Sagis *et al.* [43]. This is particularly essential when in drop/bubble oscillation experiments the interfaces are covered by crosslinked membranes with a respective macroscopic thickness rather than by a monomolecular layer [44]. As mentioned above, reliable feedback can be obtained for the applicability of PAT in such situations by analyzing the standard deviation between the calculated and experimental drop/bubble profiles [10].

### Large amplitude oscillatory dilations

First of all, large amplitude deformations of interfaces happen quite often in practice. In addition, this type of experiment is particularly suitable to visualize most relaxation mechanisms within the interfacial layer. Sagis and Fischer [45] recently summarized the use of experiments with oscillating drops or bubbles at large amplitude oscillatory dilations (LAOD) as a very efficient way to determine the interfacial dilation rheology of complex liquid interfacial layers in the non-linear visco-elastic (NLVE) regime. The standard output from PAT tensiometers yield the dilational modulus  $E_{FT}$  as evaluated from a first-harmonic Fourier transform analysis of the surface tension response. However, more detailed information about the rheological behavior of highly nonlinear visco-elastic interfacial systems remains encoded in higher harmonics [45,46]. To deal with this, a graphical method based on the analysis of Lissajous plots  $\Pi$  ( $\Delta A/A_0$ ) was proposed in Ref. [45] ( $\Pi$  is surface pressure, and  $\Delta A/A_0$  is the dimensionless amplitude of area deformation for a fixed initial surface area  $A_0$ ). The nonlinear asymmetric surface stress response  $\bar{E}$  to LAOD of an interfacial layer can be decomposed into four contributions: two pairs of large-strain ( $\bar{E}_{LE}$  and  $\bar{E}_{LC}$ ) and minimum-strain ( $\bar{E}_{ME}$  and  $\bar{E}_{MC}$ ) moduli for the regimes of expansion ( $\bar{E}_{LE}$  and  $\bar{E}_{ME}$ ) and compression ( $\bar{E}_{LC}$  and  $\bar{E}_{MC}$ ), which in turn, allow for the evaluation of a strain stiffening factor  $S$  as: 1)  $S = 0$  for linear visco-elasticity behavior; 2)  $S > 0$  for strain-hardening; and 3)  $S < 0$  for strain-softening [45]. The thus defined stiffening factor  $S$  is a measure of the degree of elastic intracycle non-linearity and can be evaluated for both regimes of dilation, namely expansion

( $S_E$ ) and compression ( $S_C$ ). Groot et al. [12] refined this approach by analyzing separately odd and even harmonics, as previously suggested by Bykov et al. [46]. The authors tested the improved methodology on complex water/air interfaces stabilized by proteins or lecithin, and provided a physical interpretation of each  $\bar{E}$ -contribution [12]. Their approach was presented in a quite general form and then applied to drop/bubble profile experiments for systems containing peptides [47], native proteins [48–50] or protein aggregates [51]. For example, in Ref. [50], LAOD was applied to  $\beta$ -lactoglobulin adsorption layers of  $H_2O/D_2O$  aqueous solutions in order to identify possible isotopic effects on the protein adsorption and rheological behavior, which is of high relevance to neutron reflectometry studies, where the usage of mixed  $H_2O/D_2O$  media is a necessary prerequisite. The experimental results did not only provide interesting interfacial rheology data but also showed that combined LAOD/dynamic surface pressure  $\Pi(t)$  measurements can be a suitable test prior to designing optimal time windows in experimental protocols for neutron reflectometry experiments. For illustration, in Figure 2 some results of LAOD experiments are shown as examples.

It is worth mentioning that the calculated values for the  $S$ -factors are quite low in magnitude (of the order of 0.1), which was found also for  $\beta$ -Lactoglobulin (BLG) at the W/O interface [52] and for other proteins at the W/A interface [12]. This means that the degree of elastic nonlinearity remains comparatively low with the increase in the relative amplitude  $\Delta A/A_0$  even of up to about 20 % [12,50].


The approach by Mielke et al. [53] is also worth mentioning as a powerful analysis of nonlinearities in the

dilation rheological behavior of fluorocarbon/hydrocarbon tetrablock amphiphiles at the water/air interface, which yields unique visco-elasticity characteristics of these interfacial layers: nonlinearities emerged even under ‘mild’ conditions, such as surface pressures of  $\Pi \approx 5$  mN/m and oscillation amplitude of only  $\Delta A/A_0 = 1$  %. Just for comparison, typical values of the amplitudes of transition to a NLVE regime for protein layers at the water/air interface are ca.  $\Delta A/A_0 = 3$ –5% [48,50] or even up to  $\approx 10\%$  [45,47].

### Depletion effects in single drop experiments


When measuring the dynamic and equilibrium surface tension of a solution drop of a strongly surface-active surfactant at low  $c$  the values differ significantly from those measured with an air bubble formed in the same solution. This effect was found much earlier and used as a tool to estimate the amount  $\Gamma$  of adsorbed proteins at the drop/bubble surface [54]. The difference is called depletion effect, as it is caused by the adsorption of surfactant at the drop surface and leads to a certain loss of concentration inside the single drop. As only emphasized recently [11], the depletion can cause large differences in the obtained adsorption layer characteristics in a quantitative analysis of experimental data. Depletion becomes significant when  $\Gamma \times A \gg c \times V$ . The volume of single drops in PAT is typically of the order of  $15 \text{ mm}^3$ , which corresponds to a drop diameter of about  $2r = 3 \text{ mm}$ . When taking spherical geometry as a rough approximation for a drop, we get  $V/A = r/3$ , so that we obtain  $V/A \approx 0.0005 \text{ cm}$ . Thus, for surfactants adsorbing significantly at  $c = 10^{-6} \text{ mol/l}$ , we obtain the condition for depletion of  $\Gamma \gg 5 \times 10^{-11} \text{ mol/cm}^2$ , which is the case for almost all proteins and also for many long chain

Figure 2

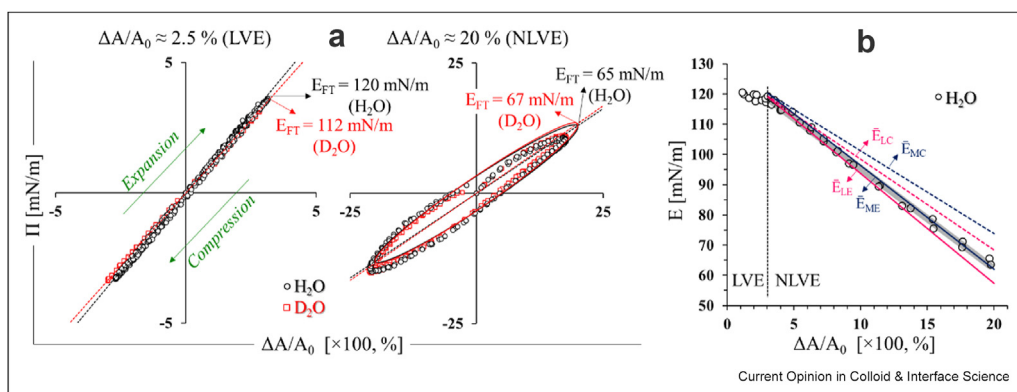

LAOD experiments at  $f = 0.1$  Hz applied to  $\beta$ -lactoglobulin adsorption layers at the water/air interface (pH 7, 10 mM phosphate buffer). **(a)** Lissajous plots  $\Pi$  vs.  $(\Delta A/A_0)$  at a steady state ( $\Pi \approx 20$  mN/m) for solutions in  $H_2O$  or  $D_2O$  for two amplitudes in the linear (LVE) and nonlinear (NLVE) visco-elasticity regime. The straight lines through the origin (0,0) are the long axes of the elliptical contours obtained from first-harmonic Fourier transform analysis (examples are shown on the right-hand side panel); the evaluated values for  $E_{FT}$  are depicted in the graphs. **(b)** Evaluated dilational modulus  $E$  vs.  $\Delta A/A_0$  for  $H_2O$ ; symbols are experimental  $E_{FT}$  and the gray-shaded ribbon is a linear regression through the data in the NLVE regime; lines are linear regressions for the moduli  $\bar{E}_{LE}$ ,  $\bar{E}_{ME}$ ,  $\bar{E}_{LC}$ , and  $\bar{E}_{MC}$ . Adapted with permission from Gochev et al. [50]. Copyright 2024 American Chemical Society.

Figure 3

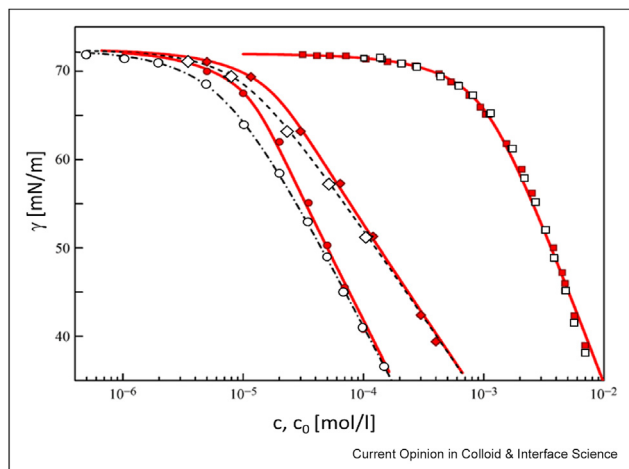

Surface tension isotherms for solutions of SDS in pure water (■□), in water with addition of 0.5 mol/l NaCl (◆◇), and for C<sub>10</sub>OH in pure water (●○); open symbols measured with bubbles formed in the solution and closed symbols measured with solution drops; further details are given in the text, according to Ref. [11]. SDS, sodium dodecyl sulfate.

surfactants. In Ref. [11], data for a number of surfactants were analyzed and one example is shown in Figure 3. As one can see, the surface tension isotherms for a surfactant like sodium dodecyl sulfate measured with single solution drops and in addition with a bubble in the surfactant solution (no depletion because the ratio V/A is typically 3 orders of magnitude larger than for a single drop) are identical. The same surfactant in 0.5 mol/l NaCl shows already measurable differences (at low *c*) between the “drop” and “bubble” data, and for decanol, the differences are already enormous.

Depletion due to adsorption effects at the surface of single solution drops has not only a strong impact on dynamic and equilibrium surface/interfacial tensions but also on the visco-elasticities of interfacial adsorption layers when measured with single oscillating drops [55]. The impact of depletion effects on the dilational interfacial visco-elasticity was shown, for example, in studies of Akanno *et al.* [56] on mixed adsorption layers of polymers and surfactants. In Ref. [57] it is shown how this complicates the data analysis so that it is recommended to use bubbles instead of drops in PAT experiments, as long as drops cannot be avoided, like in studies at liquid/liquid interfaces.

## Conclusions

Simple set-ups for drop profile analysis tensiometry can suffer from a lower accuracy, but via the combination with artificial intelligence, for example the approach proposed recently in Ref. [15], this experimental tool can provide a manifold of data with a sufficiently high precision. Still, high-end instruments will keep their

leading role in the characterization of fluid interfaces due to their great number of available complex experimental protocols and additional features like temperature and drop/bubble size control.

New experimental protocols allow for accurate measurements not only of interfacial tension but also of the dilational visco-elasticity at high pressure and high temperature. It was also shown that for particular systems, the use of PAT can lead to erroneous results, for example when the drop bulk contains sedimenting particles or the surface is covered by a kind of membrane rather than a monomolecular adsorption layer. In such cases, the analysis of the standard deviation (STD) as a measure for the deviation of the experimental from the calculated profile, helps to decide whether PAT is applicable or leads to systematic errors. Recently, PAT-STD analysis has also been developed as a novel methodology for recognition of complex layer formation, and transformation of regular adsorbed layers to membrane-like film formation.

For the future use of PAT as a routine tensiometry method, it is recommended to find the most suitable size of the drop/bubble, and to check if the important conditions for the method – homogeneous bulk and isotropic surface layer are fulfilled. In any case, we can expect that the fields of application of PAT will further grow and provide a large amount of data that give us insights into molecular processes inside the bulk of surfactant/protein solutions as well as those happening at the interface.

## Declaration of competing interest

During the preparation of this work the authors did not use any type of artificial intelligence.

The authors of this manuscript declare to have no conflicts of interest. The Ms has been submitted only to this journal and all supporting institutions are mentioned.

## Data availability

No data was used for the research described in the article.

## Acknowledgements

This work was funded by ESA via the MAP project “Emulsion Dynamics and Droplet Interfaces (EDDI)”, 4000128643/19.

## References

Papers of particular interest, published within the period of review, have been highlighted as:

- \* of special interest
- \*\* of outstanding interest

1. Bashforth F, Adams C: *An attempt to test the theories of capillary action*. Cambridge University Press; 1883. ISBN-101296997464.
2. Andreas JM, Hauser EA, Tucker WB: **Boundary tension by pendant drops**. *J Phys Chem* 1938, **42**:1001–1019, <https://doi.org/10.1021/j100903a002>.

3. Rotenberg Y, Boruvka L, Neumann AW: **Determination of surface tension and contact angle from the shapes of axisymmetric fluid interfaces.** *J Colloid Interface Sci* 1983, **93**: 169–183, [https://doi.org/10.1016/0021-9797\(83\)90396-X](https://doi.org/10.1016/0021-9797(83)90396-X).
4. Chen P, Kwok DY, Prokop RM, del Rio Ol, Susnar SS, Neumann AW: **Axisymmetric drop shape analysis (ADSA) and its applications.** In *Drops and bubbles in interfacial research*. Edited by Möbius D, Miller R, *Studied in interface science*, vol. 6. Amsterdam: Elsevier; 1998:61–138. ISBN: 0 444 82894 X.
5. Benjamins J, Cagna A, Lucassen-Reynders EH: **Viscoelastic properties of triacylglycerol/water interfaces covered by proteins.** *Colloids Surf A* 1996, **114**:245–254, [https://doi.org/10.1016/0927-7757\(96\)03533-9](https://doi.org/10.1016/0927-7757(96)03533-9).
6. Chen H, Muros-Cobos JL, Holgado-Terriza JA, Amirfazli A: **Surface tension measurement with a smartphone using a pendant drop.** *Colloids Surf A* 2017, **533**:213–217, <https://doi.org/10.1016/j.colsurfa.2017.08.019>.
7. Huang YH, Frostad JM: **A new instrument for interfacial dilatation rheology.** *Rev Sci Instrum* 2023, **94**, 115108, <https://doi.org/10.1063/5.0168137>.
8. Berry JD, Neeson MJ, Dagastine RR, Chan DYC, Tabor RF: **Measurement of surface and interfacial tension using pendant drop tensiometry.** *J Colloid Interface Sci* 2015, **454**: 226–237, <https://doi.org/10.1016/j.jcis.2015.05.012>.
9. Yang J, Yu K, Zuo YY: **Accuracy of axisymmetric drop shape analysis in determining surface and interfacial tensions.** *Langmuir* 2017, **33**:8914–8923, <https://doi.org/10.1021/acs.langmuir.7b01778>.
- This work analysis the situation in PAT with respect to the optimum size of drops or bubbles required for most accurate experiments. While Berry et al. [8] favor the Worthington number, in contrast to the most often applied Bond number, the authors propose a new dimensionless number, the Neumann number, which has obviously some advantages as it contains the optimum radius and height of the drop/bubble.
10. Mahmoudvand M, Vatanparast H, Javadi A, Kantzas A, Burns S, Dolgos M, Miller R, Bahramian A: **Evaluation of interfacial structure of self-assembled nanoparticle layers: use of standard deviation between calculated and experimental drop profiles as a novel method.** *Langmuir* 2024, **40**: 2130–2145, <https://doi.org/10.1021/acs.langmuir.3c03081>.
- The method of PAT is often applied to liquid–fluid interface, although the basic conditions are not fulfilled, such as a homogeneous surface layer (isotropic interfacial tension) and a homogeneous bulk phase. Remarkable deviations of the standard deviation (difference between the experimental and calculated profiles) over the classical values of  $\pm 1 \mu\text{m}$  point at the fact that the profiles cannot adequately be described by the GLE and hence, the application of PAT leads to significant errors – i.e. only apparent values for the interfacial tension and related quantities are obtained.
11. Kairaliyeva T, Aksenenko EV, Mucic N, Makievski AV, Fainerman VB, Miller R: **Surface tension and adsorption studies by drop profile analysis tensiometry.** *J Surfactants Deterg* 2017, **20**:1225–1241, <https://doi.org/10.1007/s11743-017-2016-y>.
- When single drops of low-concentrated surfactant or protein solutions are studied with PAT, the initial bulk concentration is reduced during the process of interfacial layer formation due to adsorption of molecules at the drop surface. Thus, after the adsorption equilibrium has been reached, the surface layer is in equilibrium with a bulk phase of a lower concentration, hence the isotherm of equilibrium interfacial tension data must be constructed as a function of the equilibrium rather than initial concentrations.
12. de Groot A, Yang J, Sagis LMC: **Surface stress decomposition in large amplitude oscillatory interfacial dilatation of complex interfaces.** *J Colloid Interface Sci* 2023, **638**:569–581, <https://doi.org/10.1016/j.jcis.2023.02.007>.
13. Dowlati S, Javadi A, Miller R, Eckert K, Kraume M: **Unfolding lipase at interfaces studied via interfacial dilatation rheology: the impact of urea.** *Colloids Interfaces* 2022, **6**:56, <https://doi.org/10.3390/colloids6040056>.
14. Ashoorian S, Javadi A, Hosseinpour N, Nassar NN: **Interrelationship of bulk and oil-water interfacial properties of asphaltenes.** *J Mol Liq* 2023, **381**, 121761, <https://doi.org/10.1016/j.molliq.2023.121761>.
15. Kratz FS, Kierfeld J: **Pendant drop tensiometry: a machine learning approach.** *J Chem Phys* 2020, **153**, 094102, <https://doi.org/10.1063/5.0018814>.
16. Hyer AP, McMillin RE, Ferri JK: **The shape of things to come: axisymmetric drop shape analysis using deep learning.** *J Colloid Interface Sci* 2024, **653**:1188–1195, <https://doi.org/10.1016/j.jcis.2023.09.120>.
- The application of PAT, particularly under dynamic conditions, requires fast data handling. The introducing a machine learning-based approach into the analysis of drop/bubble images becomes significantly accelerated, and the accuracy increased. The approach also provides great support in respect to image qualities, i.e. even under bad experimental conditions, often happening with technical systems or field studies, accurate results can be obtained.
17. Zamora JM, Marquez R, Forgiarini AM, Langevin D, Salager JL: **Interfacial rheology of low interfacial tension systems using a new oscillating spinning drop method.** *J Colloid Interface Sci* 2018, **519**:27–37, <https://doi.org/10.1016/j.jcis.2018.02.015>.
18. Delahaije RJB, Sagis LMC, Yang J: **Impact of particle sedimentation in pendant drop tensiometry.** *Langmuir* 2022, **38**: 10183–10191, <https://doi.org/10.1021/acs.langmuir.2c01193>.
19. Wojciechowski K, Borucka K, Mierzejewska J: **Are all yeast biosurfactants really capable of lowering surface tension below 30 mN/m?** *Colloids Surf B Biointerfaces* 2023, **230**, 113503, <https://doi.org/10.1016/j.colsurfb.2023.113503>.
- The study demonstrates in an excellent way how incorrect experimental conditions, such as the presence of unexpected or ignored emulsions in a liquid system, can lead to well established but wrong ideas about the constant surface tension of yeast culture media caused by respective biosurfactants. It turns out that such artifacts can be avoided by respective handling of the culture media before starting any measurements.
20. Tang H, Cheng X: **Measurement of liquid surface tension by fitting the lying droplet profile.** *Measurement* 2022, **188**, 110379, <https://doi.org/10.1016/j.measurement.2021.110379>.
21. Soori T, Rassoulinejad-Mousavi SM, Zhang L, Rokoni A, Sun Y: **A machine learning approach for estimating surface tension based on pendant drop images.** *Fluid Phase Equilib* 2021, **538**, 113012, <https://doi.org/10.1016/j.fluid.2021.113012>.
22. Yu K, Yang J, Zuo YY: **Droplet oscillation as an arbitrary waveform generator.** *Langmuir* 2018, **34**:7042–7047, <https://doi.org/10.1021/acs.langmuir.8b01059>.
23. Yang J, Yu K, Tsuji T, Jha R, Zuo YY: **Determining the surface dilatation rheology of surfactant and protein films with a droplet waveform generator.** *J Colloid Interface Sci* 2019, **537**: 547–553, <https://doi.org/10.1016/j.jcis.2018.11.054>.
24. Toor A, Forth J, Bochner de Araujo S, Consiglia Merola M, Jiang Y, Liu X, Chai Y, Hou H, Ashby PD, Fuller GG, Russell TP: **Mechanical properties of solidifying assemblies of nanoparticle surfactants at the oil–water interface.** *Langmuir* 2019, **35**:13340–13350, <https://doi.org/10.1021/acs.langmuir.9b01575>.
25. Paap U, Kreß B, Steinrück HP, Maier F: **Probing surface and interfacial tension of ionic liquids in vacuum with the pendant drop and sessile drop method.** *Int J Mol Sci* 2022, **23**, 13158, <https://doi.org/10.3390/ijms232113158>.
26. Martínez-Pedrero F, Carbone C, Rubio RG, Ortega F, Guzmán E: **A critical examination of the physics behind the formation of particle-laden fluid interfaces.** *Curr Opin Colloid Interface Sci* 2024. in press.
27. Gupta A, Pandey A, Kesarwani H, Sharma S, Saxena A: **Automated determination of interfacial tension and contact angle using computer vision for oil field applications.** *J Petrol Explor Prod Technol* 2022, **12**:1453–1461, <https://doi.org/10.1007/s13202-021-01398-6>.
28. Argyri SM, Evenäs L, Bordes R: **Contact-free measurement of surface tension on single droplet using machine learning and acoustic levitation.** *J Colloid Interface Sci* 2023, **640**:637–646, <https://doi.org/10.1016/j.jcis.2023.02.077>.
29. Fu Y, Chen Y, Zhang C, Lei Y, Liu X: **Prediction surface tension of ionic liquid–water mixtures using a hybrid group contribution and artificial neural network method.** *Fluid Phase Equilib* 2023, **563**, 113571, <https://doi.org/10.1016/j.fluid.2022.113571>.



30. Mohan M, Smith MD, Demerdash O, Kidder MK, Smith JC: **Predictive understanding of the surface tension and velocity of sound in ionic liquids using machine learning.** *J Chem Phys* 2023, **158**, 214502, <https://doi.org/10.1063/5.0147052>.
31. Barrabino A, Holt T, Bjørkvik B, Lindeberg E: **First approach to measure interfacial rheology at high-pressure conditions by the oscillating drop technique.** *Colloids Interfaces* 2021, **5**:23, <https://doi.org/10.3390/colloids5020023>.
- Although dynamic interfacial tensions can be measured by PAT at elevated temperatures and pressures for quite some time, the authors demonstrate impressively that a respective design also allows for drop oscillations that give access to the dilational visco-elasticity of the liquids to be studied.
32. Bjørkvik BJA: **What is the correct interfacial tension between methane and water at high-pressure/high-temperature conditions?** *Fluid Phase Equilib* 2023, **572**, 113834, <https://doi.org/10.1016/j.fluid.2023.113834>.
33. Føyen T, Brattekkås B, Fernø MA, Barrabino A, Holt T: **Increased CO<sub>2</sub> storage capacity using CO<sub>2</sub>-foam.** *Int J Greenh Gas Control* 2020, **96**, 103016, <https://doi.org/10.1016/j.ijggc.2020.103016>.
34. Ricci E, Giuranno D, Sobczak N: **Further development of testing procedures for high temperature surface tension measurements.** *J Mater Eng Perform* 2013, **22**:3381–3388, <https://doi.org/10.1007/s11665-013-0624-x>.
- The article presents a PAT setup based on pendant drops for the study of surface tensions of liquid metals and alloys at high temperatures. This configuration allows for minimizing effects of reactivity of the molten alloys with the container at the higher temperature.
35. Ricci E, Amore S, Giuranno D, Novakovic R, Tuissi A, Sobczak N, Nowak R, Korpala B, Bruzda G: **Surface tension and density of Si-Ge melts.** *J Chem Phys* 2014, **140**, 214704, <https://doi.org/10.1063/1.4879775>.
36. Tseng WC, Tsay RY, Le TTY, Hussain S, Noskov BA, Akentiev A, Yeh HH, Lin SY: **Evaluation of the dilational modulus of protein films by pendant bubble tensiometry.** *J Mol Liq* 2022, **349**, 118113, <https://doi.org/10.1016/j.molliq.2021.118113>.
37. Hussain S, Rivas JEM, Tseng WC, Tsay RY, Noskov B, Loglio G, Lin SY: **Measurement of dilational modulus of an adsorbed BSA film using pendant bubble tensiometry: from a clean interface to saturation.** *Colloids Interfaces* 2024, **8**:4, <https://doi.org/10.3390/colloids8010004>.
38. Maradiaga Rivas JE, Hussain S, Tseng WC, Noskov B, Lin SY: **A study on the dilational modulus of adsorbed globular protein films – under a near periodic area fluctuation and rapid surface perturbation.** *J Taiwan Inst Chem Eng* 2024, **155**, 105288, <https://doi.org/10.1016/j.jtice.2023.105288>.
39. Leser ME, Acquistapace S, Cagna A, Makievski AV, Miller R: **Limits of oscillation frequencies in drop and bubble shape tensiometry.** *Colloids Surf A* 2005, **261**:25–28, <https://doi.org/10.1016/j.colsurfa.2004.11.043>.
40. Karbaschi M, Bastani D, Javadi A, Kovalchuk VI, Kovalchuk NM, Makievski AV, Bonaccorso E, Miller R: **Drop profile analysis tensiometry under highly dynamic conditions.** *Colloids Surf A* 2012, **413**:292–297, <https://doi.org/10.1016/j.colsurfa.2012.04.027>.
41. Marquez R, Bullon J, Forgiarini A, Salager JL: **The oscillatory spinning drop technique. An innovative method to measure dilational interfacial rheological properties of brine-crude oil systems in the presence of asphaltenes.** *Colloids Interfaces* 2021, **5**:42, <https://doi.org/10.3390/colloids5030042>.
- The spinning drop method is of particular importance for measurements at very low interfacial tensions. This is in particular important in oil recovery studies. The authors demonstrate how this methodology can be refined such that even harmonic interfacial compressions and expansions can be generated to get access to the dilational visco-elasticity of the interfacial layers involved.
42. Jaensson NO, Anderson PD, Vermant J: **Computational interfacial rheology.** *J Non-Newtonian Fluid Mech* 2021, **290**, 104507, <https://doi.org/10.1016/j.jnnfm.2021.104507>.
- The authors of this article provide an overview of the computational rheology of fluid interfacial layers. This includes the derivation of stress boundary conditions in absence and presence of structured interfaces. Particular details are given for studies for oscillation experiments with drops and bubbles when the interfaces are covered by structure layers in which an isotropic interfacial tension cannot be assumed. This contribution is of great importance but not easy to read as it represents an interdisciplinary cross-over with the rheology of materials and uses partly special terminologies.
43. Sagis LMC, Humblet-Hua KNP, van Kempen SEHJ: **Nonlinear stress deformation behavior of interfaces stabilized by food-based ingredients.** *J Phys Condens Matter* 2014, **26**, 464105, <https://doi.org/10.1088/0953-8984/26/46/464105>.
44. Jaensson NO, Vermant J: **Tensiometry and rheology of complex interfaces.** *Curr Opin Colloid Interface Sci* 2018, **37**: 136–150, <https://doi.org/10.1016/j.cocis.2018.09.005>.
45. Sagis LMC, Fischer P: **Nonlinear rheology of complex fluid–fluid interfaces.** *Curr Opin Colloid Interface Sci* 2014, **19**:520–529, <https://doi.org/10.1016/j.cocis.2014.09.003>.
46. Bykov AG, Liggieri L, Noskov BA, Pandolfini P, Ravera F, Loglio G: **Surface dilational rheological properties in the nonlinear domain.** *Adv Colloid Interface Sci* 2015, **222**:110–118, <https://doi.org/10.1016/j.cis.2014.07.006>.
47. Carbonell-Aviñó F, Clegg PS: **Non-linear dilational rheology of liquid-liquid interfaces stabilized by dipeptide hydrogels.** *Rheol Acta* 2023, **62**:45–55, <https://doi.org/10.1007/s00397-022-01380-x>.
48. Shen P, Peng J, Sagis LMC, Landman J: **Air-water interface properties and foam stabilization by mildly extracted lentil protein.** *Food Hydrocolloids* 2024, **147**, 109342, <https://doi.org/10.1016/j.foodhyd.2023.109342>.
49. Ikenaga N, Sagis LMC: **Interfacial moduli at large strains and stability of emulsions stabilised by plant proteins at high bulk shear rates.** *Food Hydrocolloids* 2024, **146**, 109248, <https://doi.org/10.1016/j.foodhyd.2023.109248>.
50. Gochev G, Schneck E, Miller R: **Effects of aqueous isotopic substitution on adsorption dynamics and dilational rheology of  $\beta$ -lactoglobulin layers at the water/air interface.** *J Phys Chem B* 2024, **128**:2821–2830, <https://doi.org/10.1021/acs.jpbc.3c08417>.
51. Chen M, Sala G, Meinders MJB, van Valenberg HJF, van der Linden E, Sagis LMC: **Interfacial properties, thin film stability and foam stability of casein micelle dispersions.** *Colloids Surf B Biointerfaces* 2017, **149**:56–63, <https://doi.org/10.1016/j.colsurfb.2016.10.010>.
52. Bock A, Steinhäuser U, Drusch S: **Partitioning behavior and interfacial activity of phenolic acid derivatives and their impact on  $\beta$ -lactoglobulin at the oil-water interface.** *Food Biophys* 2021, **16**:191–202, <https://doi.org/10.1007/s11483-020-09663-7>.
53. Mielke S, Habe T, Veschgini M, Liu X, Yoshikawa K, Krafft MP, Tanaka M: **Emergence of strong nonlinear viscoelastic response of semifluorinated alkane monolayers.** *Langmuir* 2018, **34**:2489–2496, <https://doi.org/10.1021/acs.langmuir.7b03997>.
54. Makievski AV, Loglio G, Krägel J, Miller R, Fainerman VB, Neumann AW: **Adsorption of protein layers at the water/air interface as studied by axisymmetric drop and bubble shape analysis.** *J Phys Chem* 1999, **103**:9557–9561, <https://doi.org/10.1021/jp990775y>.
55. Fainerman VB, Kovalchuk VI, Aksenenko EV, Miller R: **Dilational viscoelasticity of adsorption layers measured by drop and bubble profile analysis: reason for different results.** *Langmuir* 2016, **32**:5500–5509, <https://doi.org/10.1021/acs.langmuir.6b01134>.
56. Akanno A, Guzmán E, Fernández-Peña L, Ortega F, Rubio RG: **Surfactant-like behavior for the adsorption of mixtures of a polycation and two different zwitterionic surfactants at the water/vapor interface.** *Molecules* 2019, **24**:3442, <https://doi.org/10.3390/molecules24193442>.
57. Kovalchuk VI, *et al.*: **Visco-elasticity of surfactant interfacial layers.** *Curr Opin Colloid Interf Sci* 2024. in press.